

# Light Measurement Report

Print date: 19-12-2024

Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](#)

Operator:



## Laboratory and Equipment

Laboratory Owner and Location  
Goniospectrometer System and Type  
Sensor Name, Calibr. Date and Serial No.  
Spectrometer Manufacturer and Model

Viso Systems, Copenhagen V, Denmark  
LabSpion – Type C, horizontal  
LabSensor Model2 – 11-1-2024 – 3130191315  
Ibsen Photonics, Denmark – Freedom VIS (Custom Viso)

## Measurement Conditions

Number of C-planes and Resolution  
 $\gamma$  (gamma)-Resolution  
Test Distance  
Input Power, Power and Displ. Factors  
Input RMS Voltage and Current  
Frequency of Input Power  
Warm-up Time and Variation

12 planes – 30°  
5°  
7,71 m  
7,3 W – PF 0,69 – DPF 0,73  
230 V – 0,046 A  
50 Hz  
Not completed – 2,0%

## Tested Light Source




Product Name  
Item No. and Manufacturer  
Product Description (line 1)

808198-ROOD  
808198-ROOD – Dutchfulfillment  
BACK-LIT LED PANEEL | DOVER | 60x60CM | RGB+CCT | 40W

## Main Light Measurement Results

Output – Total Lumen (Up% / Down%)  
Efficiency  
Peak Intensity and Beam Angle  
Correlated Color Temperature, Target/Measured  
Color Rendering Index  
Color Rendering TM30-18  
Color Shift, CIE duv and MacAdam Steps  
Flicker

161 lm – 2,48% / 97,52%  
22 lm/W  
52,4 cd – 115,5°  
CCT = 0 K / 0 K  
CRI 0,0  
 $R_f$  0,0 –  $R_g$  0,0  
Duv n/a – SDCM n/a  
SVM 0 – PstLM 0,03

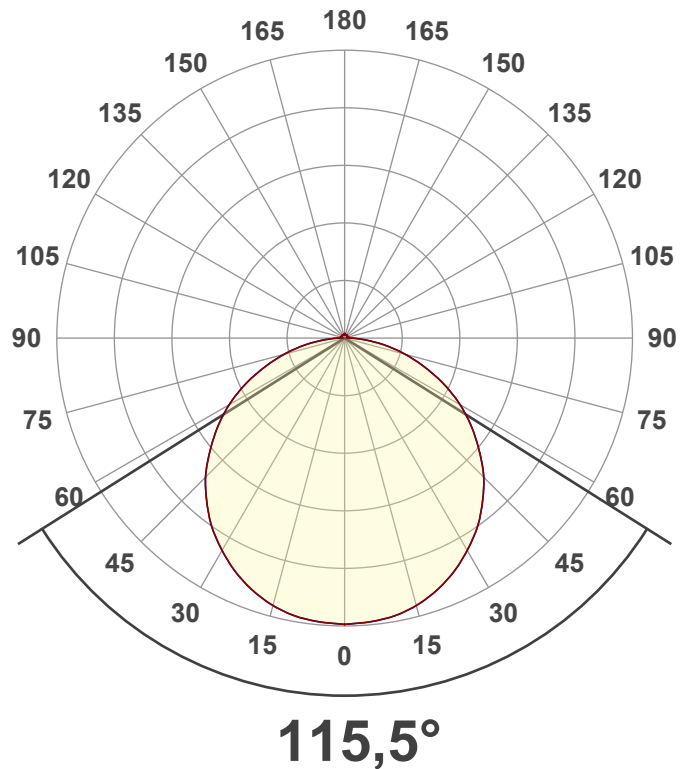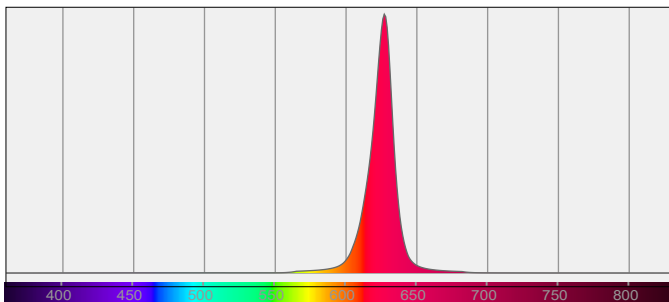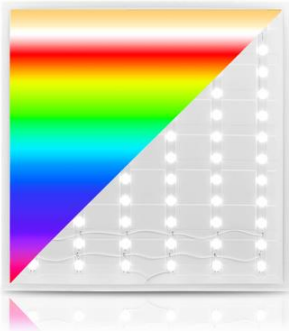

# Light Measurement Report

Print date: 19-12-2024

Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS


Measurement tracking No. and Link: [VT241219-005510](#)

Operator:



## Luminous Intensity diagram

Unit: 0-100% of peak intensity

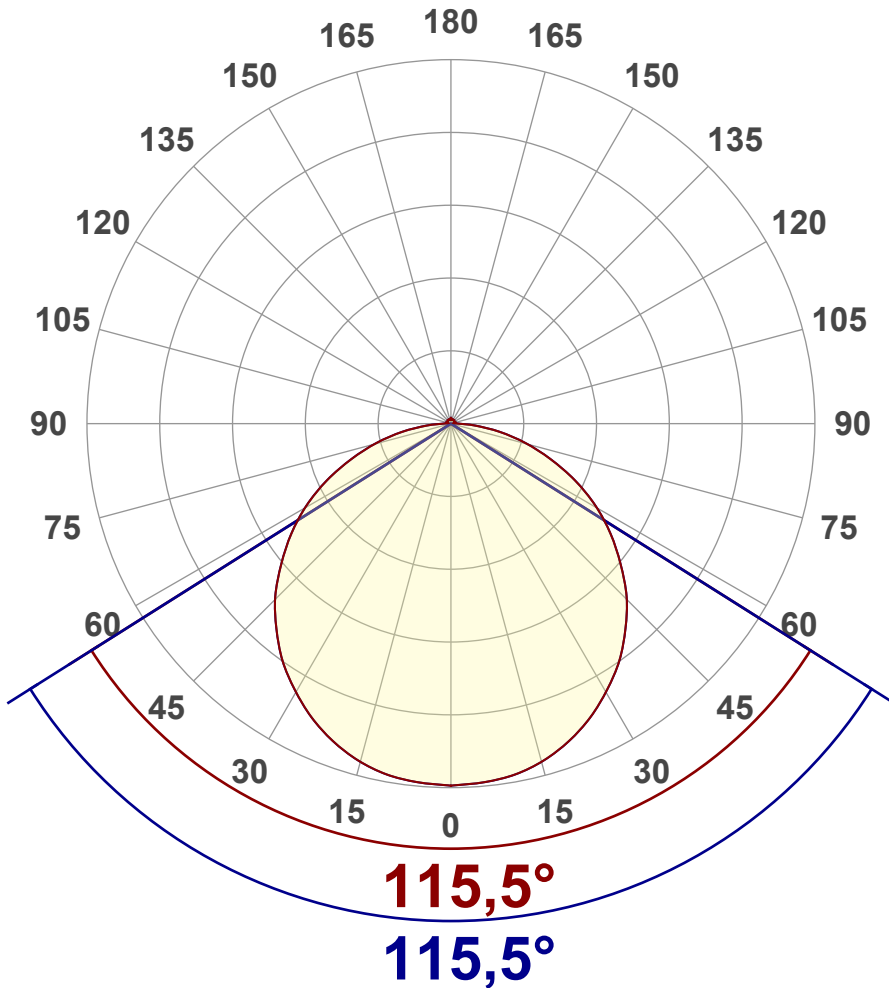

## Main Values

Output (total Lumen)	161 lm
Lumen Up% / Down%	2,48% / 97,52%
Peak Intensity	52,4 cd
Beam Angle (50%)	115,5°
Beam Angle (90%)	115,5°
Beam Angle (10%)	115,5°

## Cut-off Angle

Average 2,5%	179,7°
--------------	--------

## Field Angle

Average 10%	166,1°
-------------	--------


## Intensity Ratio

In 120° cone	74,9%
In 90° cone	50,6%

**C000-C180**

**C090-C270**

## Linear distribution diagram - Intensity (candela) vs $\gamma$ -angle

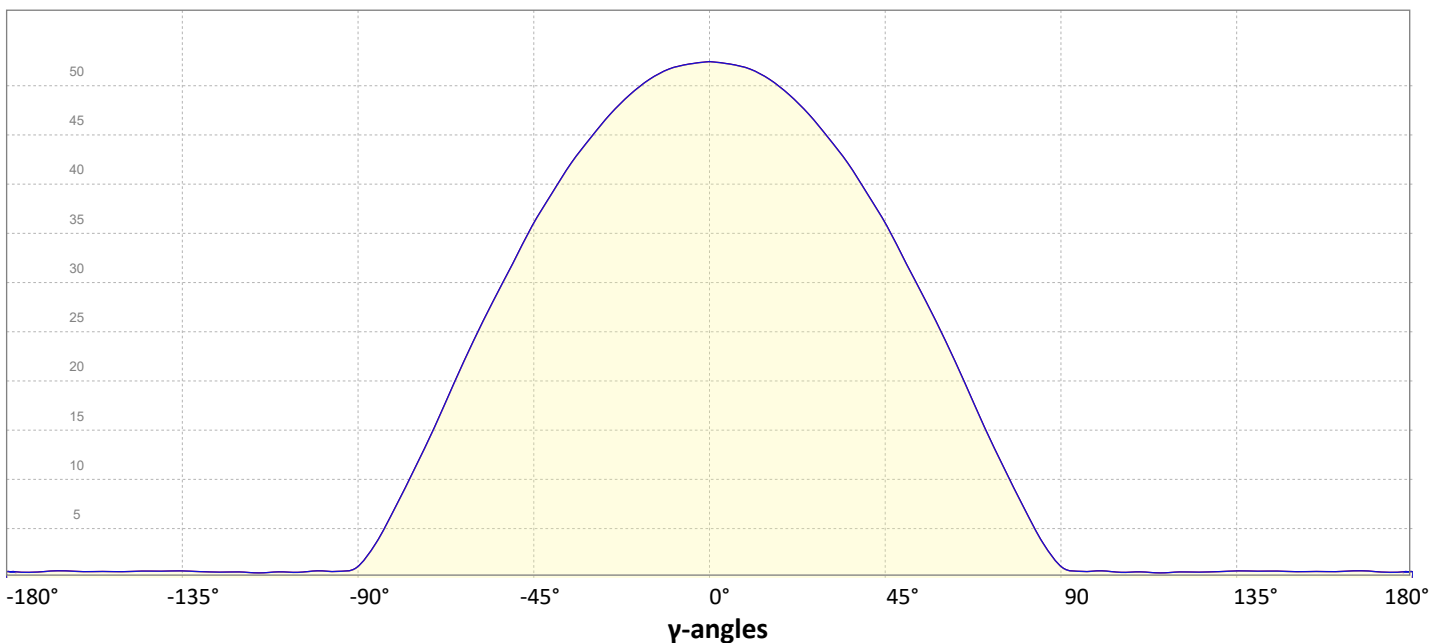

# Light Measurement Report

Print date: 19-12-2024


Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](https://www.viso-systems.com/VT241219-005510)

Operator:




## Iso-intensity Diagram (Iso-candela)

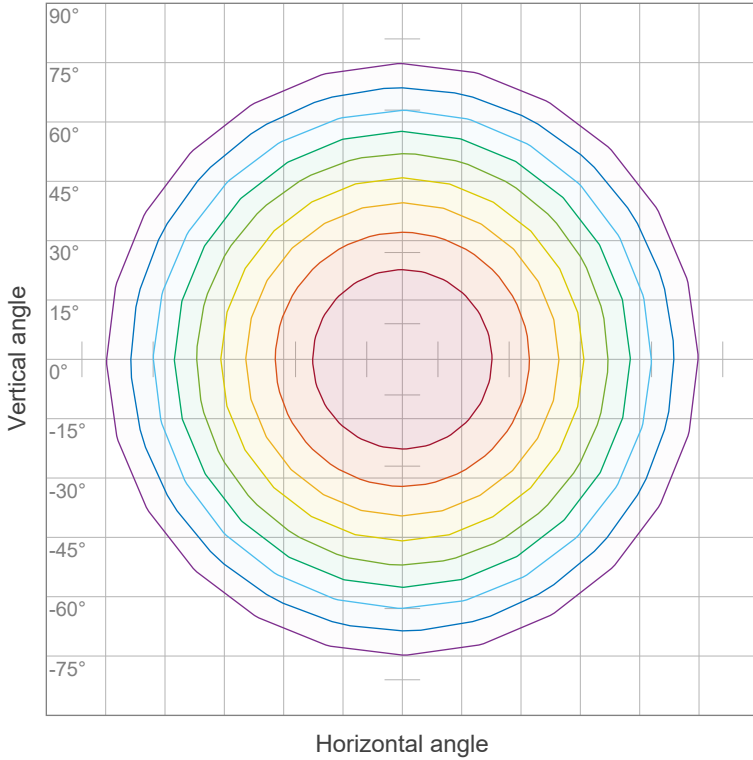

90 %	47,2 cd
80 %	41,9 cd
70 %	36,7 cd
60 %	31,5 cd
50 %	26,2 cd
40 %	21,0 cd
30 %	15,7 cd
20 %	10,5 cd
10 %	5,2 cd

Peak intensity: 52,4 cd  
Number of c-planes: 12

## Iso-illuminance Diagram (Iso-lux)

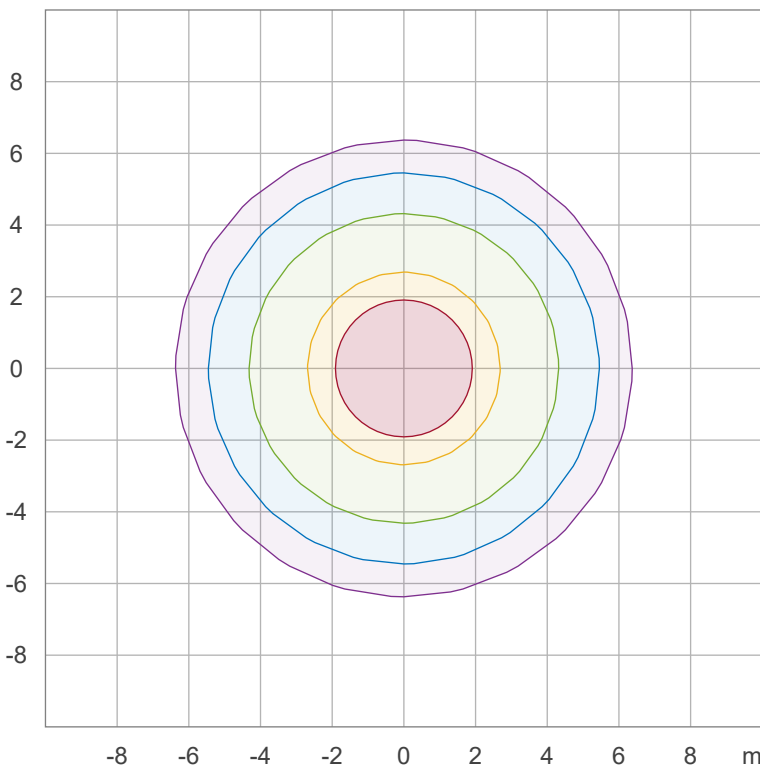

50,0 %	2,9 lx
30,0 %	1,7 lx
10,0 %	0,6 lx
5,0 %	0,3 lx
3,0 %	0,2 lx

Peak illuminance: 5,8 lx  
Mounting height: 3,0 m  
Number of c-planes: 12



# Light Measurement Report

Print date: 19-12-2024


Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](https://www.viso-systems.com/VT241219-005510)

Operator:



## Beam Details

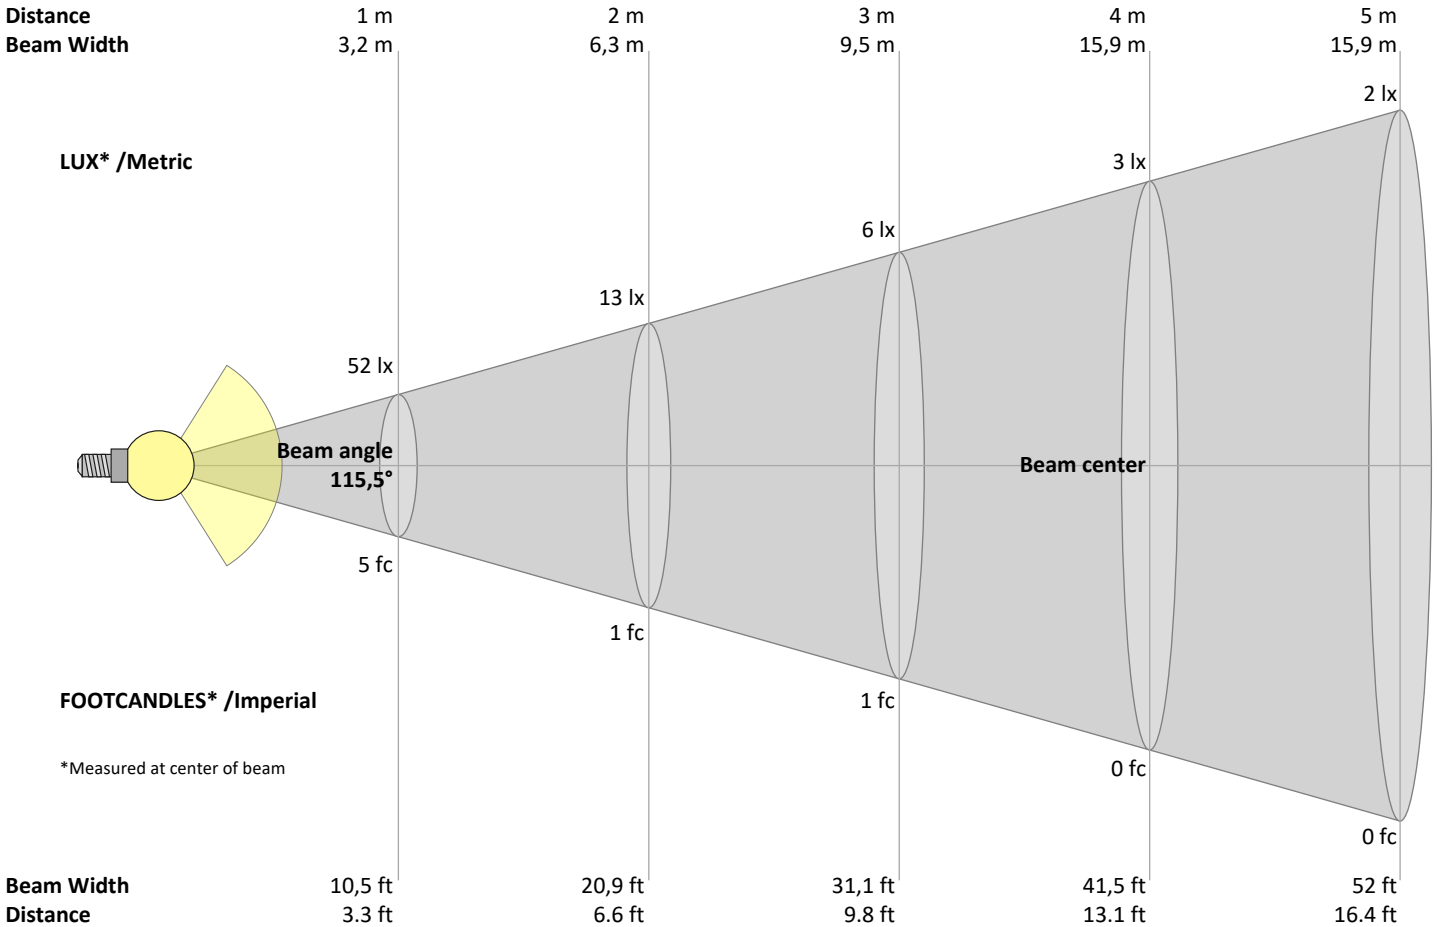

### Beam intensities from 1 – 20 m

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	m	
3,3	6,6	9,8	13,1	16,4	19,7	23	26,2	29,5	32,8	36,1	39,4	42,7	45,9	49,2	52,5	55,8	59,1	62,3	65,6	ft	
52	13	6	3	2	1	1	1	1	1	0	0	0	0	0	0	0	0	0	0	0	lux
4,9	1,2	0,5	0,3	0,2	0,1	0,1	0,1	0,1	0	0	0	0	0	0	0	0	0	0	0	0	fc

### Intensities in 0° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
52,4	52,2	51,7	50,7	49,2	47,3	44,9	42,3	39,3	36,0	32,2	28,4	24,4	20,1	15,7	11,5	7,5	3,8	1,2	0,7	cd
100%	100%	99%	97%	94%	90%	86%	81%	75%	69%	61%	54%	47%	38%	30%	22%	14%	7%	2%	1%	of 0°val

### Intensities in 90° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
52,4	52,2	51,7	50,7	49,2	47,3	44,9	42,3	39,3	36,0	32,2	28,4	24,4	20,1	15,7	11,5	7,5	3,8	1,2	0,7	cd
100%	100%	99%	97%	94%	90%	86%	81%	75%	69%	61%	54%	47%	38%	30%	22%	14%	7%	2%	1%	of 0°val

### Intensities in 180° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
52,4	52,2	51,7	50,7	49,2	47,3	44,9	42,3	39,3	36,0	32,2	28,4	24,4	20,1	15,7	11,5	7,5	3,8	1,2	0,7	cd
100%	100%	99%	97%	94%	90%	86%	81%	75%	69%	61%	54%	47%	38%	30%	22%	14%	7%	2%	1%	of 0°val

### Intensities in 270° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
52,4	52,2	51,7	50,7	49,2	47,3	44,9	42,3	39,3	36,0	32,2	28,4	24,4	20,1	15,7	11,5	7,5	3,8	1,2	0,7	cd
100%	100%	99%	97%	94%	90%	86%	81%	75%	69%	61%	54%	47%	38%	30%	22%	14%	7%	2%	1%	of 0°val

# Light Measurement Report

Print date: 19-12-2024

Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](#)

Operator:



## Light Planning – UGR table

Uncorrected, comprehensive UGR table according to 117-1995

Reflectances		70	70	50	50	30	70	70	50	50	30
	ρ Ceiling	70	70	50	50	30	70	70	50	50	30
	ρ Walls	50	30	50	30	30	50	30	50	30	30
	ρ Floor	20	20	20	20	20	20	20	20	20	20
Room size		Viewed Crosswise					Viewed Endwise				
H = mounting height above eye level		(Viewing direction orthogonal to lamp length axis)					(Viewing direction parallel to lamp length axis)				
X	Y										
2H	2H	6,1	7,3	6,4	7,7	7,9	6,1	7,3	6,4	7,7	7,9
	3H	7,6	8,9	8,1	9,2	9,5	7,6	8,9	8,1	9,2	9,5
	4H	8,3	9,5	8,8	9,9	10,2	8,3	9,5	8,8	9,9	10,2
	6H	9,0	10,0	9,3	10,3	10,8	9,0	10,0	9,3	10,3	10,8
	8H	9,2	10,2	9,5	10,5	11,0	9,2	10,2	9,5	10,5	11,0
	12H	9,3	10,3	9,7	10,7	11,2	9,3	10,3	9,7	10,7	11,2
4H	2H	6,7	7,9	7,2	8,2	8,5	6,7	7,9	7,2	8,2	8,5
	3H	8,6	9,6	9,0	10,0	10,4	8,6	9,6	9,0	10,0	10,4
	4H	9,3	10,3	9,8	10,7	11,3	9,3	10,3	9,8	10,7	11,3
	6H	10,0	10,9	10,5	11,3	11,7	10,0	10,9	10,5	11,3	11,7
	8H	10,3	11,1	10,8	11,5	11,9	10,3	11,1	10,8	11,5	11,9
	12H	10,5	11,1	11,0	11,6	12,1	10,5	11,1	11,0	11,6	12,1
8H	4H	9,6	10,4	10,2	10,9	11,3	9,6	10,4	10,2	10,9	11,3
	6H	10,5	11,1	11,0	11,6	12,2	10,5	11,1	11,0	11,6	12,2
	8H	10,9	11,4	11,4	12,0	12,7	10,9	11,4	11,4	12,0	12,7
	12H	11,2	11,6	11,8	12,2	12,8	11,2	11,6	11,8	12,2	12,8
12H	4H	9,7	10,3	10,2	10,8	11,3	9,7	10,3	10,2	10,8	11,3
	6H	10,6	11,1	11,2	11,7	12,4	10,6	11,1	11,2	11,7	12,4
	8H	11,0	11,5	11,6	12,0	12,7	11,0	11,5	11,6	12,0	12,7

### Variations with the observer position for the luminaire spacings, S:

S = 1.0H	0,1 / -0,1	0,1 / -0,1
S = 1.5H	0,1 / -0,2	0,1 / -0,2
S = 2.0H	0,3 / -0,4	0,3 / -0,4

## Coefficients of Utilization

Ceiling reflectance	80			70			50			30			10			0		
Wall reflectance	70	50	30	10	70	50	30	10	50	30	10	50	30	10	50	30	10	0
Floor reflectance	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	0
RCR	(RCR: Room Cavity Ratio) Room Values are expressed as percentage of Lumen delivered to the task surface																	
0	118	118	118	118	115	115	115	115	110	110	105	105	105	100	100	100	98	
1	108	103	98	94	105	100	96	92	95	92	89	91	88	86	87	85	83	80
2	98	89	82	76	95	87	80	75	83	77	73	79	75	71	76	72	69	66
3	89	78	70	63	86	76	68	62	73	66	61	70	64	59	67	62	58	56
4	81	69	60	53	79	67	59	53	65	57	52	62	56	51	59	54	50	47
5	75	61	52	46	72	60	52	45	58	50	44	55	49	44	53	48	43	41
6	69	55	46	40	67	54	46	39	52	44	39	50	43	38	48	42	38	36
7	64	50	41	35	62	49	41	35	47	40	34	46	39	34	44	38	33	31
8	59	46	37	31	58	45	37	31	43	36	31	42	35	30	40	34	30	28
9	55	42	33	28	54	41	33	28	40	33	27	38	32	27	37	31	27	25
10	52	39	31	25	50	38	30	25	37	30	25	36	29	25	35	29	24	23

# Light Measurement Report

Print date: 19-12-2024

Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](#)


Operator:



## Luminaire budgetary diagram

Uncorrected, comprehensive UGR table according to 117-1995

LAMPS (number of lamps)

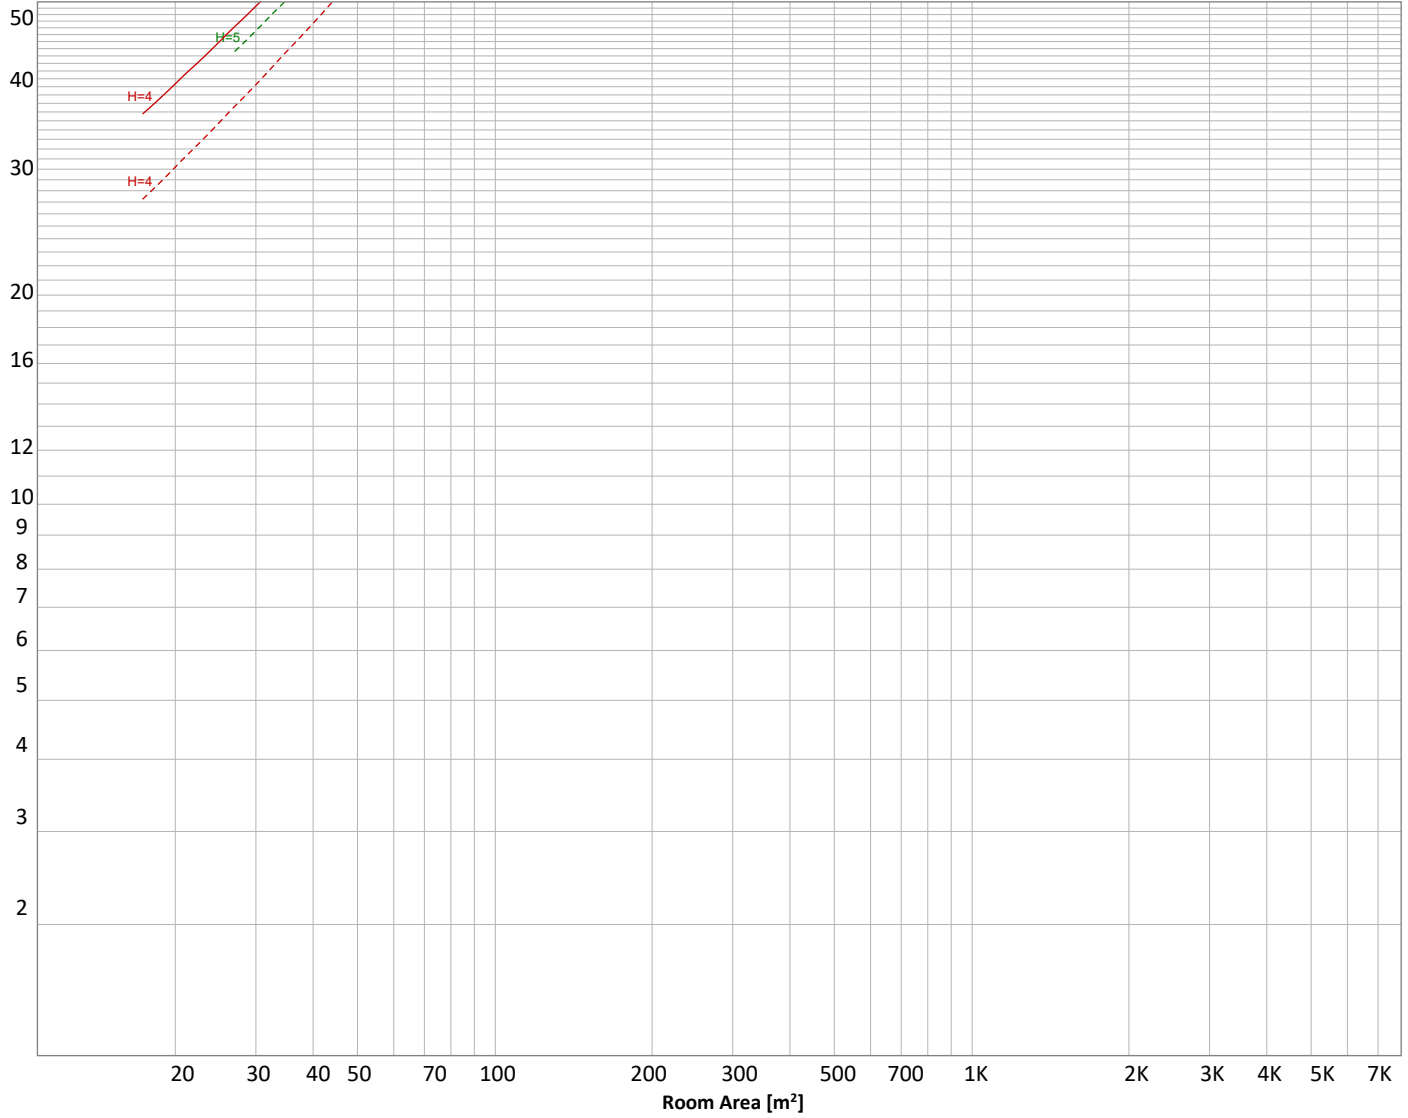

### Conditions

H = Room height	Flux = 161 lm				
H <sub>down</sub> = Lamp distance from ceiling =	0.00 m	Line type	Ceiling reflectance	ρ(%) Wall reflectance	Floor reflectance
H <sub>work</sub> = Work area height from floor =	0.00 m	-----	70	50	30
E <sub>work</sub> = Average lux on work area =	100 lx	_____	50	30	20

### Zonal Lumen Summary

0°-10°	10°-20°	20°-30°	30°-40°	40°-50°	50°-60°	60°-70°	70°-80°	80°-90°
4,97 lm	14,3 lm	21,8 lm	26,5 lm	27,7 lm	25,4 lm	19,9 lm	12,2 lm	4,43 lm
90°-100°	100°-110°	110°-120°	120°-130°	130°-140°	140°-150°	150°-160°	160°-170°	170°-180°
0,837 lm	0,637 lm	0,534 lm	0,523 lm	0,514 lm	0,414 lm	0,290 lm	0,189 lm	0,056 lm

# Light Measurement Report

Print date: 19-12-2024

Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](#)

Operator:



## Outdoor Light Planning

### Lumen per Zone

Zone (γ)	Lumen	% Total
0-10°	{LUM00-10} lm	#VALUE!
10-20°	{LUM10-20} lm	#VALUE!
20-30°	{LUM20-30} lm	#VALUE!
30-40°	{LUM30-40} lm	#VALUE!
40-50°	{LUM40-50} lm	#VALUE!
50-60°	{LUM50-60} lm	#VALUE!
60-70°	{LUM60-70} lm	#VALUE!
70-80°	{LUM70-80} lm	#VALUE!
80-90°	{LUM80-90} lm	#VALUE!
90-100°	{LUM90-100} lm	#VALUE!
100-110°	{LUM100-110} lm	#VALUE!
110-120°	{LUM110-120} lm	#VALUE!
120-130°	{LUM120-130} lm	#VALUE!
130-140°	{LUM130-140} lm	#VALUE!
140-150°	{LUM140-150} lm	#VALUE!
150-160°	{LUM150-160} lm	#VALUE!
160-170°	{LUM160-170} lm	#VALUE!
170-180°	{LUM170-180} lm	#VALUE!
Total	0 lm	#VALUE!

### Intensity peaks

Max intensity	{PEAK} cd
Intensity, 90°	{INT90} cd
Intensity, 0°	{INT0} cd

### Zonal Lumen summary


Zone (γ)	Lumen	% Total
0-30°	{LUM00-30} lm	#VALUE!
0-40°	{LUM00-40} lm	#VALUE!
0-60°	{LUM00-60} lm	#VALUE!
60-90°	{LUM60-90} lm	#VALUE!
70-100°	{LUM70-100} lm	#VALUE!
90-120°	{LUM90-120} lm	#VALUE!
0-90°	{LUM00-90} lm	#VALUE!
90-180°	{LUM90-180} lm	#VALUE!
0-180°	{LUM00-180} lm	#VALUE!

### BUG rating

	Lumen	% Total
<b>Forward light</b>		
Low(0-30°)	{BUG0} lm	#VALUE!
Medium(30-60°)	{BUG1} lm	#VALUE!
High(60-80°)	{BUG2} lm	#VALUE!
Very high(80-90°)	{BUG3} lm	#VALUE!
<b>Back light</b>		
Low(0-30°)	{BUG4} lm	#VALUE!
Medium(30-60°)	{BUG5} lm	#VALUE!
High(60-80°)	{BUG6} lm	#VALUE!
Very high(80-90°)	{BUG7} lm	#VALUE!
<b>Uplight</b>		
Low(90-100°)	{BUG8} lm	#VALUE!
High(100-180°)	{BUG9} lm	#VALUE!

## IESNA TM-15-07 Luminaire Classification System For Outdoor Luminaires

BUG rating B0 U1 G0

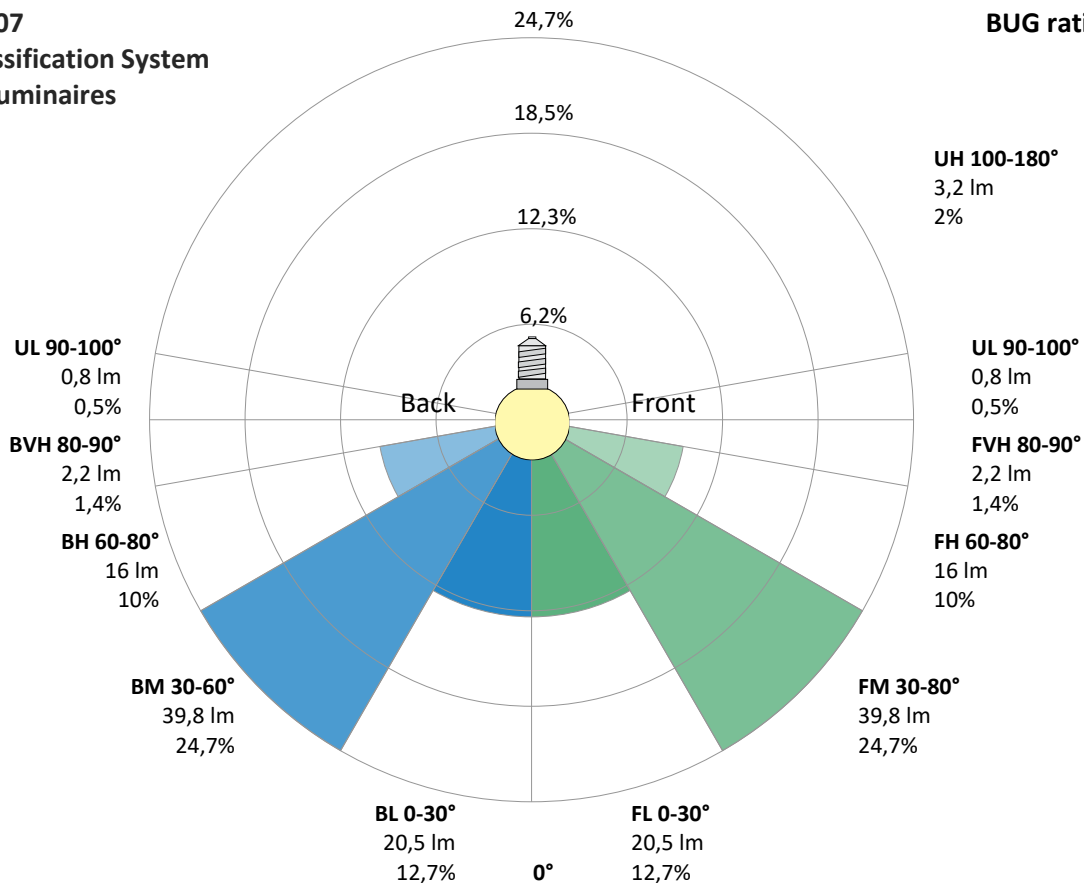

# Light Measurement Report

Print date: 19-12-2024

Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](#)

Operator:




## Power Details

### Input Power

Power feed to light source	7,3 W
Frequency of input power	50 Hz
RMS Input voltage feed, $V_{RMS}$	230 V
RMS Input current feed, $I_{RMS}$	0,046 A
Volt-Ampere or apparent power = $V_{RMS} * I_{RMS}$	10,65 VA
Displacement factor of AC power feed	0,73
Power factor of AC current feed	0,69
Total harmonic distortion of the current	35,15%
Total harmonic distortion of the voltage	0,08%

### Input Power Curve

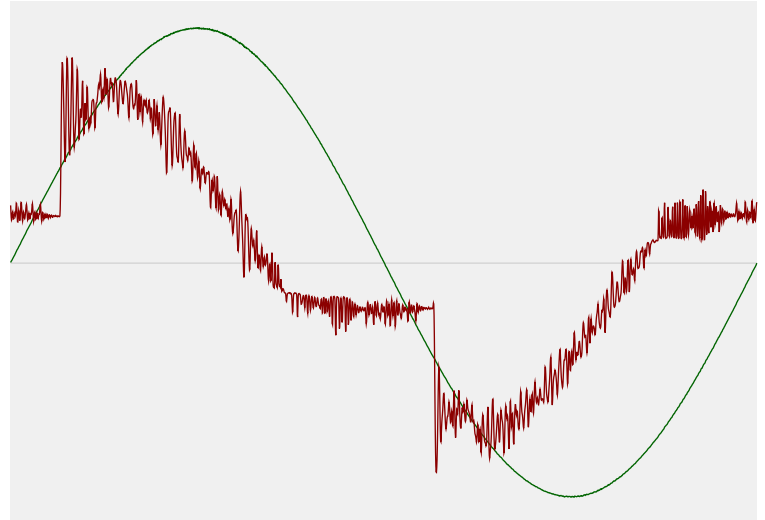

### Efficiency

Radiated power efficiency	9,9%
<div style="width: 9.9%; height: 15px; background-color: red; margin-bottom: 5px;"></div> <div style="width: 90.1%; height: 15px; background-color: gray; margin-bottom: 5px;"></div>	
Lumen efficiency	22 lm/W
<div style="width: 22%; height: 15px; background-color: orange; margin-bottom: 5px;"></div> <div style="width: 78%; height: 15px; background-color: gray; margin-bottom: 5px;"></div>	

## Stabilization Details

### Warmup Conditions

Stable period	15 min
Stable change max	2,0%
Minimum time	15 min

### Color Temperature Change

CCT start	0 K
CCT shift	0 K
CCT end	0 K


### Warmup Result

Total warmup time	Not completed
Warmup variation	+0,7%

### Output Change

Output start	160 lm
Output change	+1 lm
Output end	161 lm

### Stabilization Curve

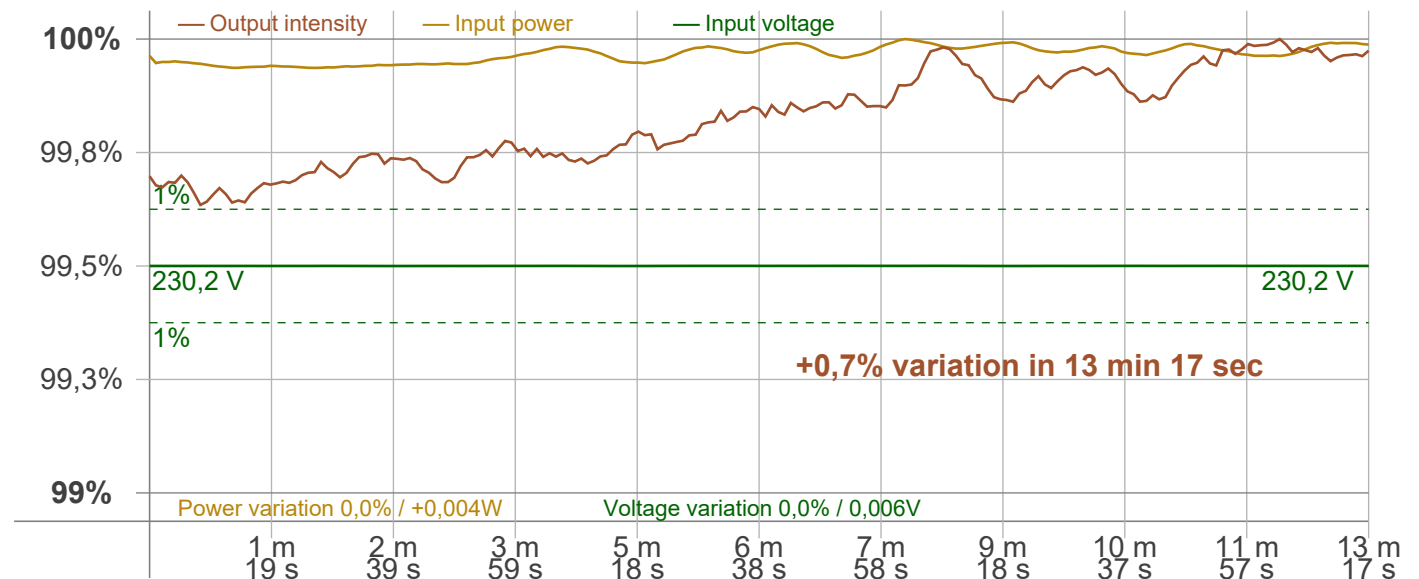

# Light Measurement Report

Print date: 19-12-2024

Measurement date and time: 19-12-2024 11:03:51 – Measurement no. VFR-241219-2597-MS

Measurement tracking No. and Link: [VT241219-005510](https://www.viso-systems.com/VT241219-005510)

Operator:



## Flicker /TLA details

Flicker Meter Type: Viso Systems LabFlicker  
 Frequency of input power: 50 Hz  
 Flicker/TLA sample rate: 20000 samples/s

**Measurement time**  
 PstLM: 180 sec  
 All other indices: 1,2 sec

### Flicker indices according to Illuminating Engineering Society (IES)

Flicker frequency: 10000 Hz  
 Percent Flicker: 9,38 %  
 Flicker index: 0,01

### Flicker indices according to California Energy Commission (CEC) 2016b

JA8/10 40 Hz: 0,11 %  
 JA8/10 90 Hz: 0,24 %  
 JA8/10 200 Hz: 0,49 %  
 JA8/10 400 Hz: 1,03 %  
 JA8/10 1000 Hz: 2,36 %


### TLA indices (re IEC TR 61547-1, IEC 61000-3-3 and IEC 61000-4-15)

PstLM value (F < 80 Hz): 0,03  
 SVM value (80 < F < 2000 Hz): 0

### Flicker indices according to Lighting Research Center (2015)

Perception metric, Assist Mp: 0,03

### Flicker frame (frame of one flicker period in time domain)

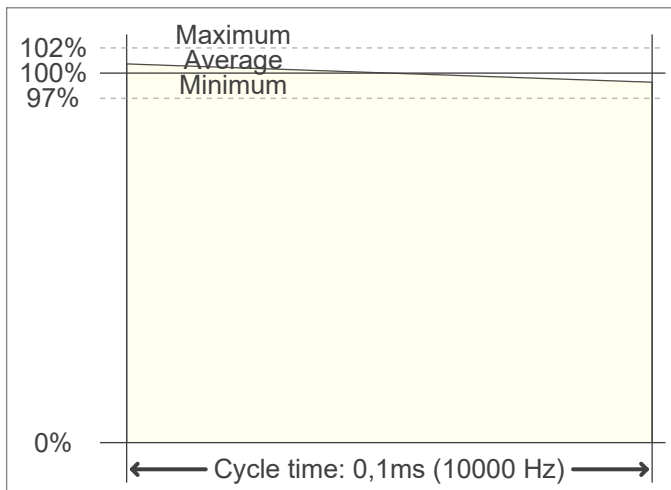

### Flicker FFT (flicker curve in frequency domain)



### IEEE 1789 Frequency/modulation plot

