

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](#)

Operator:



## Laboratory and Equipment

Laboratory Owner and Location  
Goniospectrometer System and Type  
Sensor Name, Calibr. Date and Serial No.  
Spectrometer Manufacturer and Model

Viso Systems, Copenhagen V, Denmark  
LabSpion – Type C, horizontal  
LabSensor Model2 – 11-1-2024 – 3130191315  
Ibsen Photonics, Denmark – Freedom VIS (Custom Viso)

## Measurement Conditions

Number of C-planes and Resolution  
 $\gamma$  (gamma)-Resolution  
Test Distance  
Input Power, Power and Displ. Factors  
Input RMS Voltage and Current  
Frequency of Input Power  
Warm-up Time and Variation

16 planes – 22,5°  
5°  
12,09 m  
50,4 W – PF 0,97 – DPF 0,97  
230 V – 0,227 A  
50 Hz  
Lamp stabilized in 15 min 1 sec – 2,0%

## Tested Light Source



Product Name  
Item No. and Manufacturer  
Product Description (line 1)  
35W/40W/45W/55W | ZWART | CCT SWITCH

812973-3000K-50W  
812973-3000K-50W – Dutchfulfillment  
3-FASE RAILARMATUUR | TARVOS | KANTELBAAR | 150CM |

## Main Light Measurement Results

Output – Total Lumen (Up% / Down%)  
Efficiency  
Peak Intensity and Beam Angle  
Correlated Color Temperature, Target/Measured  
Color Rendering Index  
Color Rendering TM30-18  
Color Shift, CIE duv and MacAdam Steps  
Flicker

6797 lm – 4,93% / 95,07%  
135 lm/W  
2816 cd – 91,5°  
CCT = 3000 K / 2992 K  
CRI 81,3  
 $R_f$  82,1 –  $R_g$  98,6  
Duv 0,0033 – SDCM 3,5  
SVM 0 – PstLM 0,02

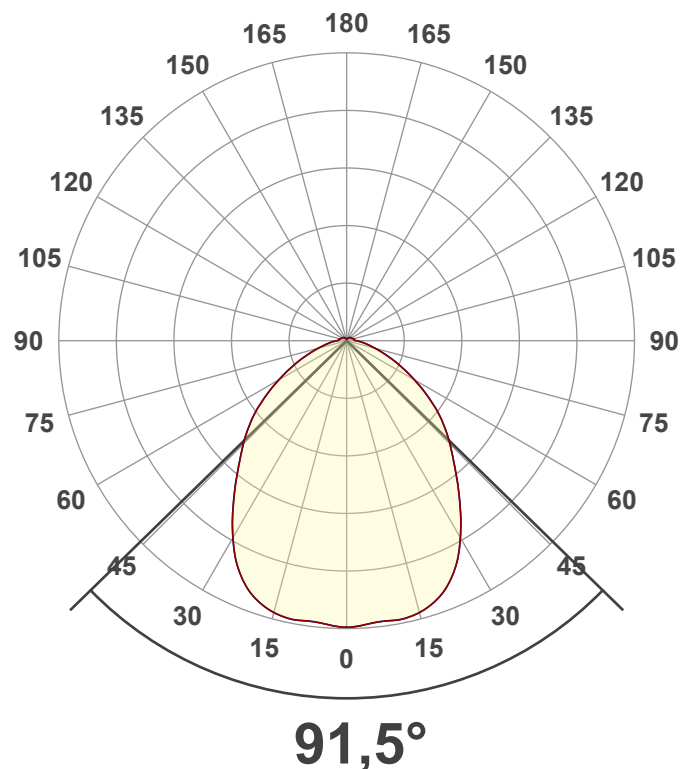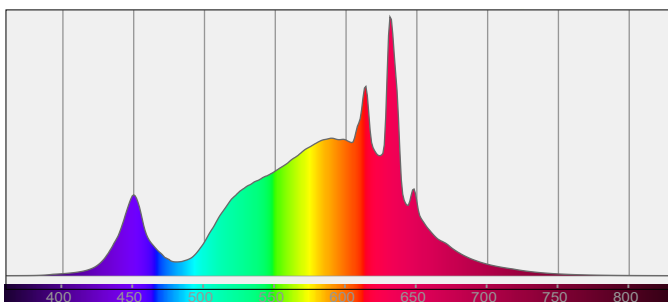

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS


Measurement tracking No. and Link: [VT251029-003886](#)

Operator:



## Luminous Intensity diagram

Unit: 0-100% of peak intensity

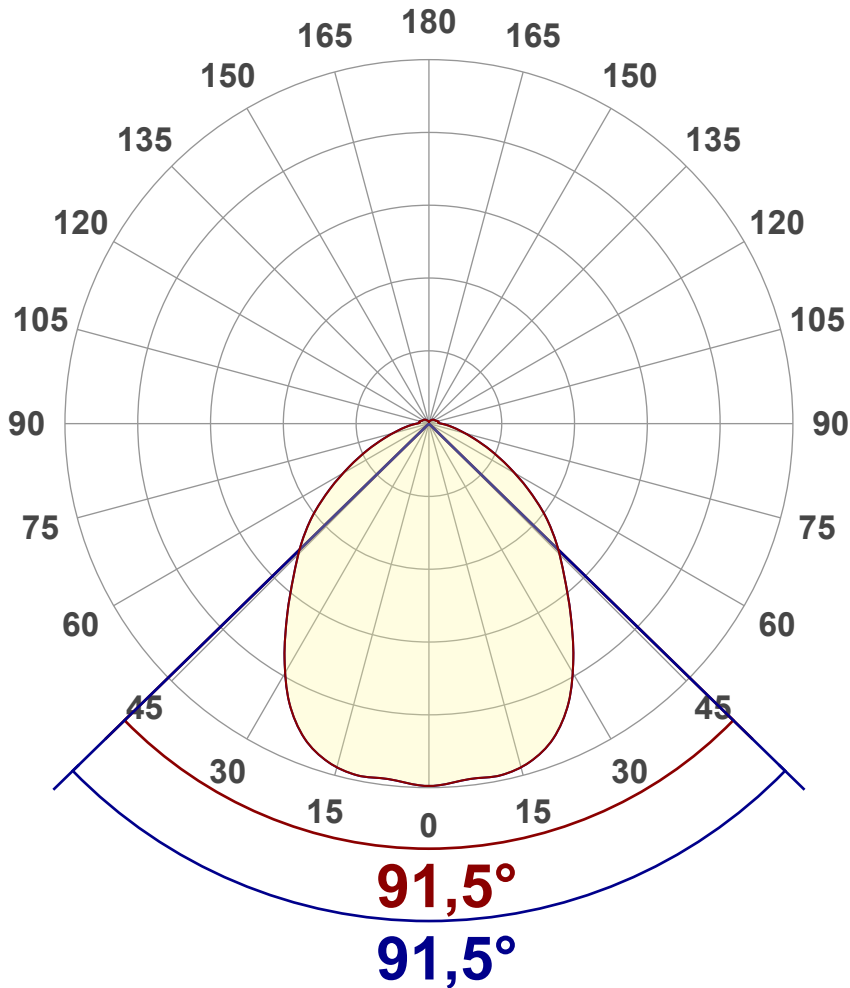

## Main Values

Output (total Lumen)	6797 lm
Lumen Up% / Down%	4,93% / 95,07%
Peak Intensity	2816 cd
Beam Angle (50%)	91,5°
Beam Angle (90%)	91,5°
Beam Angle (10%)	91,5°

## Cut-off Angle

Average 2,5%	210,6°
--------------	--------

## Field Angle

Average 10%	151,3°
-------------	--------


## Intensity Ratio

In 120° cone	79,6%
In 90° cone	58,5%

**C000-C180**

**C090-C270**

## Linear distribution diagram - Intensity (candela) vs $\gamma$ -angle

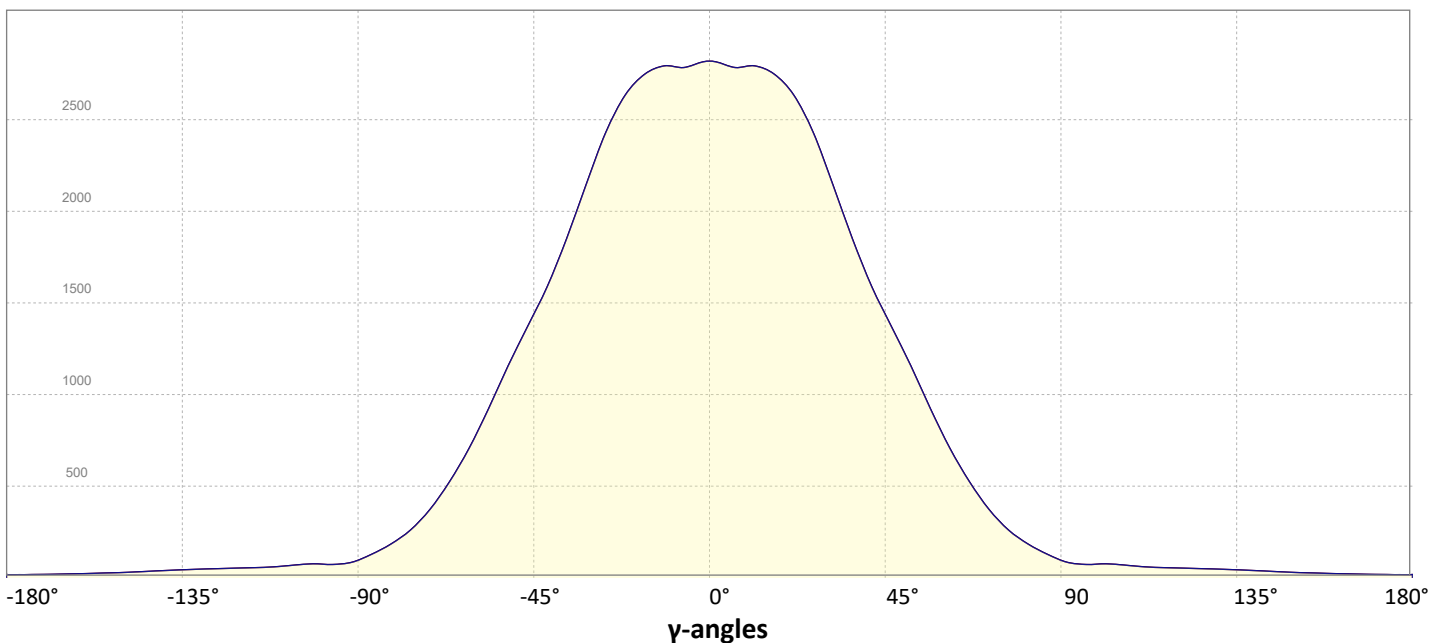

# Light Measurement Report

Print date: 29-10-2025


Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](https://www.viso-systems.com/VT251029-003886)

Operator:



## Iso-intensity Diagram (Iso-candela)

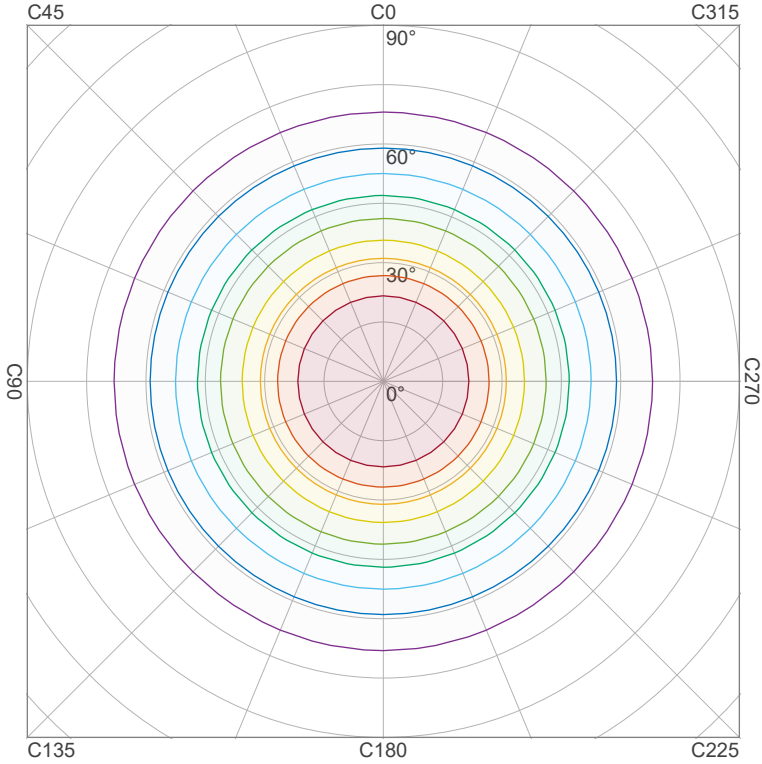


90 %	2534,2 cd
80 %	2252,7 cd
70 %	1971,1 cd
60 %	1689,5 cd
50 %	1407,9 cd
40 %	1126,3 cd
30 %	844,7 cd
20 %	563,2 cd
10 %	281,6 cd

Peak intensity: 2815,8 cd

Number of c-planes: 16

## Iso-illuminance Diagram (Iso-lux)

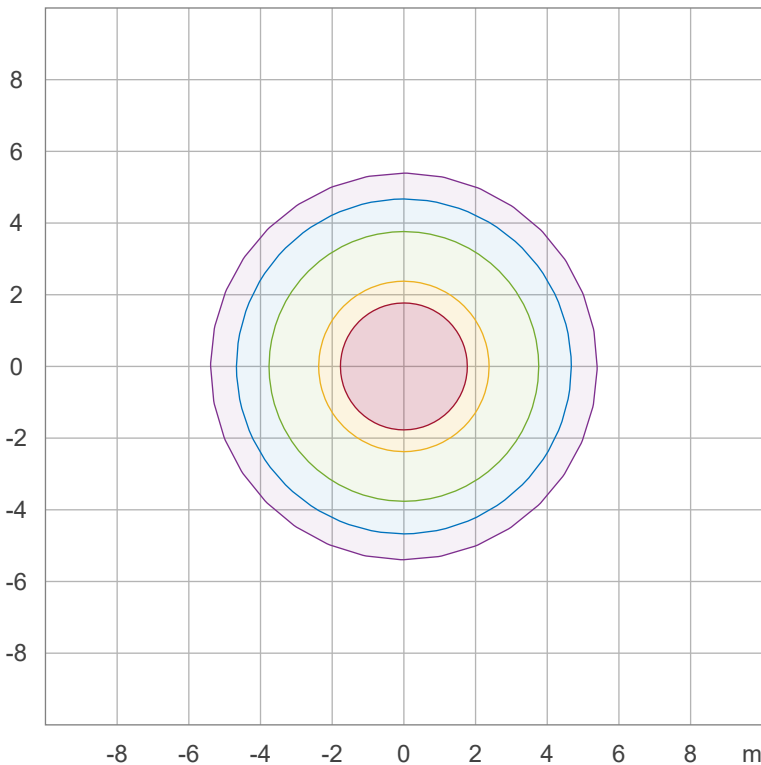

50,0 %	156,4 lx
30,0 %	93,9 lx
10,0 %	31,3 lx
5,0 %	15,6 lx
3,0 %	9,4 lx

Peak illuminance: 312,9 lx

Mounting height: 3,0 m

Number of c-planes: 16

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](#)

Operator:




## Color details

Correlated Color Temperature, Target CCT = 3000 K  
 Correlated Color Temperature, Measured CCT = 2992 K  
 Color Rendering Index CRI 81,3  
 Color Rendering Index, R9 (red component) R9 = 17,2  
 Color Rendering TM30-18 R<sub>f</sub> 82,1 – R<sub>g</sub> 98,6  
 Color Quality Scale CQS = 80,7

MacAdam Steps SDCM = 3,5  
 Color coordinates CIE 1931 (x;y) = (0,437;0,404)  
 Color coordinate CIEs 1960 (u;v) = (0,251;0,348)  
 Color deviation from BBL Duv = 0,0033  
 Color coordinate CIEs 1976 (CIELUV) (u';v') = (0,251;0,521)


### CIE 1931

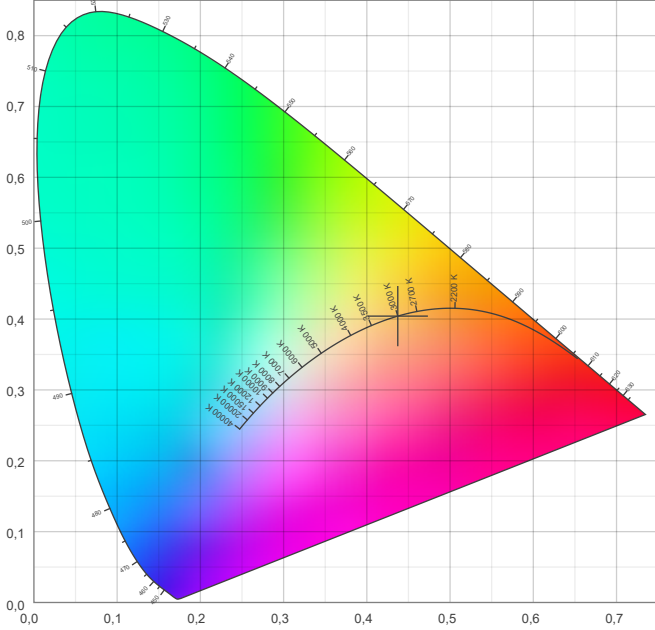

### CIE 1931 – zoomed on Planckian locus




### Color Rendering Index per reference color (CIE 1995)

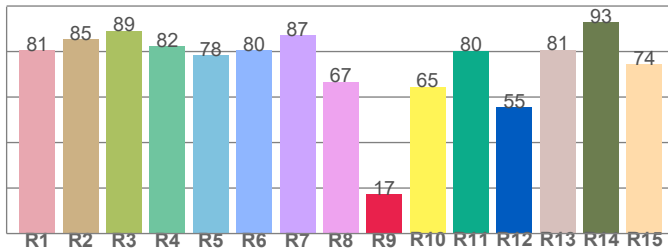


CRI R values, only R1-R8 are used to calculate final CRI value

R1	R2	R3	R4	R5	R6	R7	R8	R9	R10	R11	R12	R13	R14	R15
80,6	85,4	89,2	82,3	78,4	80,5	87,2	66,6	17,2	64,6	80,3	55,5	80,8	92,9	74,4

### Spectral power distribution (SPD) / W/nm – 0-100%

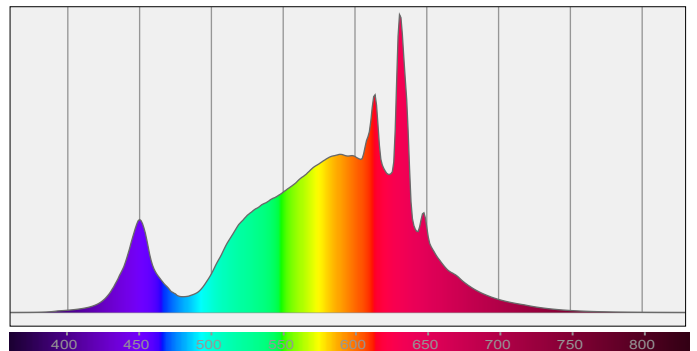


### TM30-18 R<sub>f</sub>-values per hue bin

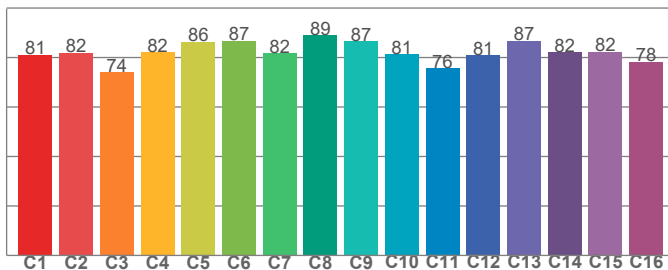

TM30 C values, 16 binned values out of total of 99 C values

C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
81,1	81,9	74,0	82,1	86,3	86,8	81,7	89,1	86,6	81,3	75,7	81,0	86,7	82,1	82,3	78,4

### Color Quality Scale by reference color

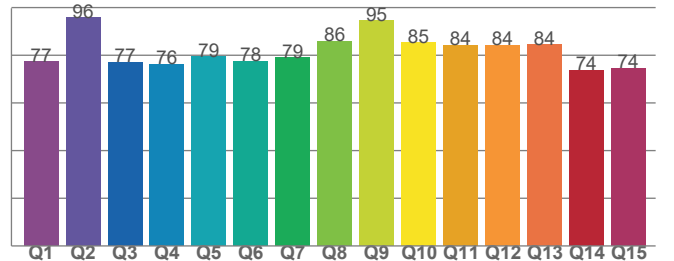

CQS Q values

Q1	Q2	Q3	Q4	Q5	Q6	Q7	Q8	Q9	Q10	Q11	Q12	Q13	Q14	Q15
77,3	95,7	77,0	76,2	79,4	77,5	79,0	85,9	94,5	85,2	84,1	84,1	84,5	73,7	74,5

# Light Measurement Report

Print date: 29-10-2025


Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](https://www.viso-systems.com/VT251029-003886)

Operator:



## Beam Details

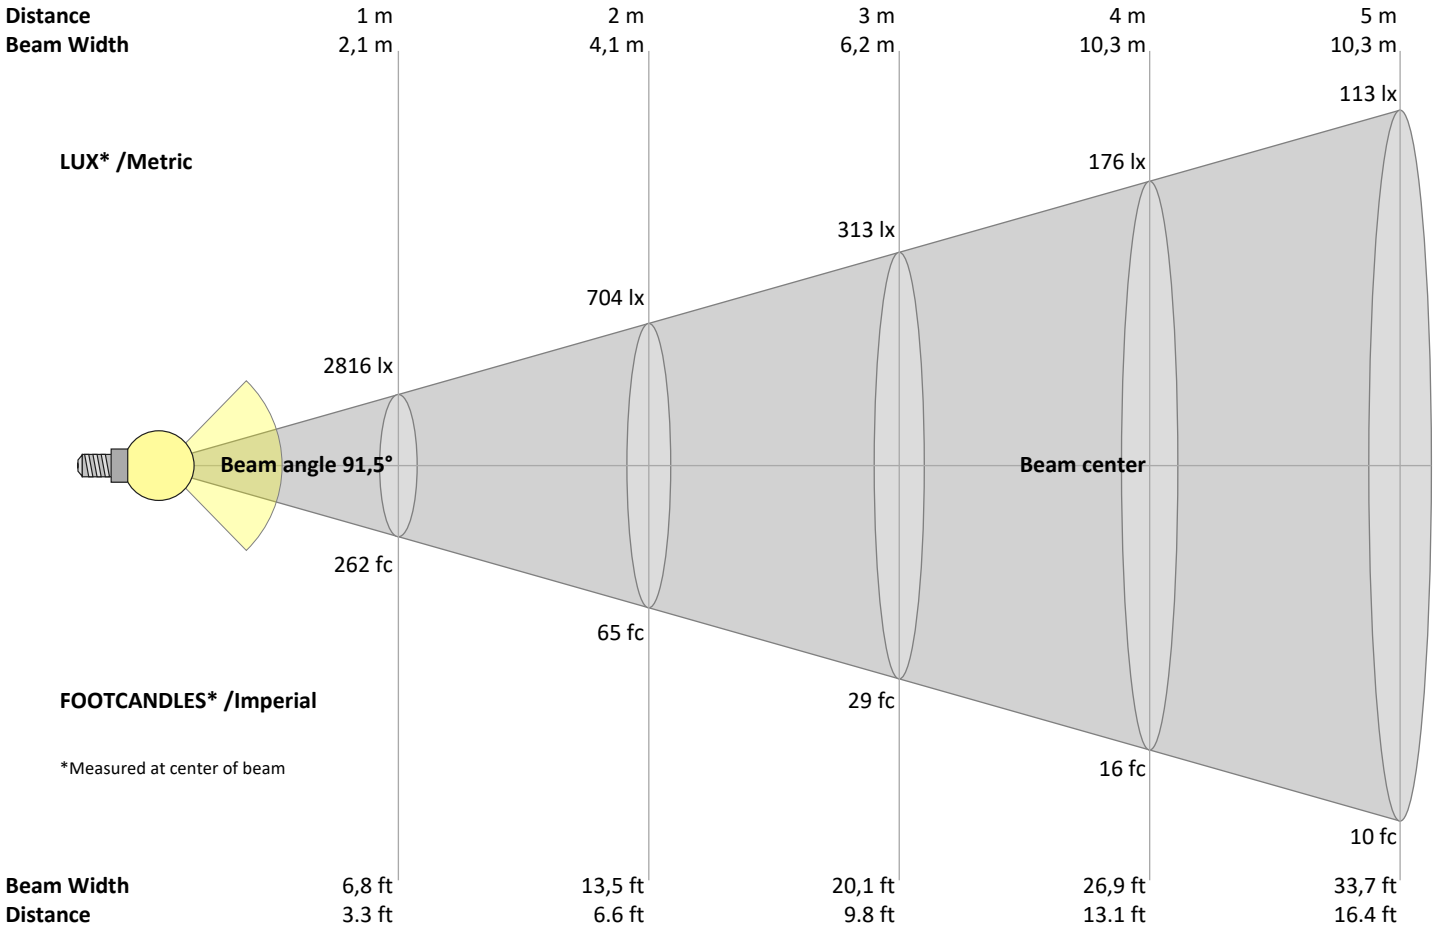

### Beam intensities from 1 – 20 m

1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	m
3,3	6,6	9,8	13,1	16,4	19,7	23	26,2	29,5	32,8	36,1	39,4	42,7	45,9	49,2	52,5	55,8	59,1	62,3	65,6	ft
2816	704	313	176	113	78	57	44	35	28	23	20	17	14	13	11	10	9	8	7	lux
261,6	65,4	29,1	16,3	10,5	7,3	5,3	4,1	3,2	2,6	2,2	1,8	1,5	1,3	1,2	1	0,9	0,8	0,7	0,7	fc

### Intensities in 0° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
2816	2794	2791	2763	2670	2494	2236	1944	1671	1440	1224	996	774	582	421	296	208	145	98	76	cd
100%	99%	99%	98%	95%	89%	79%	69%	59%	51%	43%	35%	28%	21%	15%	11%	7%	5%	3%	3%	of 0°val

### Intensities in 90° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
2816	2794	2791	2763	2670	2494	2236	1944	1671	1440	1224	996	774	582	421	296	208	145	98	76	cd
100%	99%	99%	98%	95%	89%	79%	69%	59%	51%	43%	35%	28%	21%	15%	11%	7%	5%	3%	3%	of 0°val

### Intensities in 180° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
2816	2794	2791	2763	2670	2494	2236	1944	1671	1440	1224	996	774	582	421	296	208	145	98	76	cd
100%	99%	99%	98%	95%	89%	79%	69%	59%	51%	43%	35%	28%	21%	15%	11%	7%	5%	3%	3%	of 0°val

### Intensities in 270° c-plane

0°	5°	10°	15°	20°	25°	30°	35°	40°	45°	50°	55°	60°	65°	70°	75°	80°	85°	90°	95°	γ
2816	2794	2791	2763	2670	2494	2236	1944	1671	1440	1224	996	774	582	421	296	208	145	98	76	cd
100%	99%	99%	98%	95%	89%	79%	69%	59%	51%	43%	35%	28%	21%	15%	11%	7%	5%	3%	3%	of 0°val

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](https://www.viso-systems.com/VT251029-003886)

Operator:



## Light Planning – UGR table

Uncorrected, comprehensive UGR table according to 117-1995

Reflectances		70	70	50	50	30	70	70	50	50	30
	ρ Ceiling	70	70	50	50	30	70	70	50	50	30
	ρ Walls	50	30	50	30	30	50	30	50	30	30
	ρ Floor	20	20	20	20	20	20	20	20	20	20
Room size		Viewed Crosswise					Viewed Endwise				
H = mounting height above eye level		(Viewing direction orthogonal to lamp length axis)					(Viewing direction parallel to lamp length axis)				
X	Y										
2H	2H	22,8	23,8	23,1	24,2	24,5	23,1	24,1	23,4	24,5	24,8
	3H	23,6	24,8	24,1	25,1	25,4	24,0	25,2	24,5	25,5	25,8
	4H	24,0	25,1	24,5	25,4	25,8	24,5	25,6	25,0	25,9	26,3
	6H	24,4	25,3	24,8	25,7	26,2	25,0	25,9	25,4	26,3	26,7
	8H	24,5	25,4	24,9	25,8	26,3	25,2	26,1	25,6	26,5	27,0
	12H	24,6	25,5	25,1	25,9	26,5	25,4	26,3	25,8	26,7	27,2
4H	2H	23,2	24,2	23,6	24,6	24,9	23,4	24,5	23,9	24,8	25,2
	3H	24,3	25,2	24,8	25,6	26,2	24,7	25,6	25,1	26,0	26,5
	4H	24,8	25,6	25,3	26,1	26,7	25,2	26,0	25,7	26,5	27,1
	6H	25,2	26,0	25,8	26,4	26,9	25,7	26,5	26,3	26,9	27,4
	8H	25,4	26,1	26,0	26,6	27,0	26,0	26,7	26,6	27,2	27,6
	12H	25,6	26,2	26,1	26,7	27,2	26,3	26,9	26,9	27,4	28,0
8H	4H	25,0	25,7	25,5	26,1	26,6	25,3	26,1	25,9	26,5	27,0
	6H	25,6	26,1	26,1	26,6	27,3	26,1	26,6	26,6	27,1	27,8
	8H	25,9	26,3	26,5	26,9	27,7	26,5	26,9	27,1	27,5	28,2
	12H	26,2	26,6	26,8	27,2	27,8	26,9	27,3	27,6	27,9	28,6
12H	4H	25,0	25,6	25,5	26,1	26,6	25,3	25,9	25,9	26,4	27,0
	6H	25,7	26,1	26,2	26,7	27,4	26,1	26,6	26,7	27,2	27,9
	8H	26,0	26,4	26,6	27,0	27,6	26,6	27,0	27,2	27,5	28,2

### Variations with the observer position for the luminaire spacings, S:

S = 1.0H	0,1 / -0,2	0,1 / -0,1
S = 1.5H	0,3 / -0,4	0,2 / -0,3
S = 2.0H	0,7 / -0,8	0,6 / -0,7

## Coefficients of Utilization

Ceiling reflectance	80			70			50			30			10			0		
Wall reflectance	70	50	30	10	70	50	30	10	50	30	10	50	30	10	50	30	10	0
Floor reflectance	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	20	0
RCR	(RCR: Room Cavity Ratio)																	
	Room Values are expressed as percentage of Lumen delivered to the task surface																	
0	118	118	118	118	115	115	115	115	108	108	108	103	103	103	98	98	98	95
1	108	104	100	96	105	101	97	94	96	93	90	91	89	87	87	85	83	81
2	99	92	85	80	96	89	84	79	85	80	76	81	77	74	77	74	71	69
3	91	81	74	68	88	79	72	67	76	70	65	72	67	63	69	65	62	59
4	84	73	65	58	81	71	64	58	68	62	56	65	60	55	63	58	54	52
5	78	66	57	51	75	64	56	50	62	55	49	59	53	48	57	52	48	45
6	72	59	51	45	70	58	50	45	56	49	44	54	48	43	52	47	42	40
7	67	54	46	40	65	53	45	40	51	44	39	49	43	39	48	42	38	36
8	63	50	42	36	61	49	41	36	47	40	35	46	39	35	44	38	34	32
9	59	46	38	33	57	45	38	32	44	37	32	42	36	32	41	35	31	29
10	55	42	35	30	54	42	35	30	40	34	29	39	33	29	38	33	29	27

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](https://www.viso-systems.com/VT251029-003886)


Operator:



## Luminaire budgetary diagram

Uncorrected, comprehensive UGR table according to 117-1995

LAMPS (number of lamps)

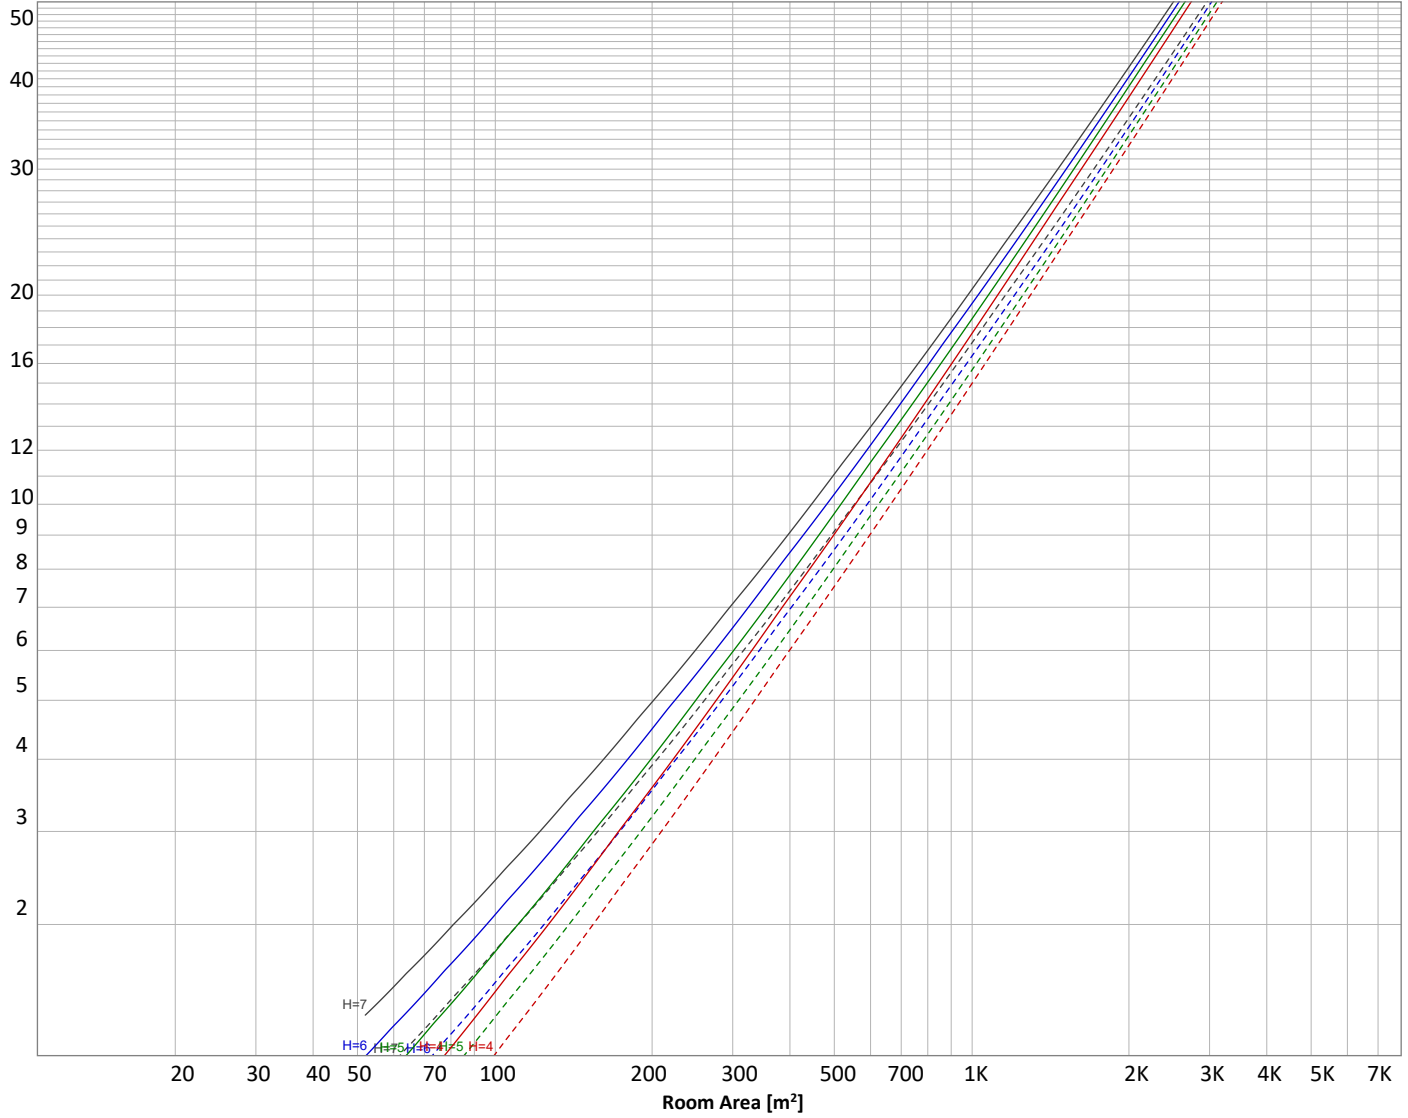

### Conditions

H = Room height	Flux = 6797 lm				
H <sub>down</sub> = Lamp distance from ceiling =	0.00 m	Line type	Ceiling reflectance	ρ(%) Wall reflectance	Floor reflectance
H <sub>work</sub> = Work area height from floor =	0.00 m	-----	70	50	30
E <sub>work</sub> = Average lux on work area =	100 lx	—————	50	30	20

### Zonal Lumen Summary

0°-10°	10°-20°	20°-30°	30°-40°	40°-50°	50°-60°	60°-70°	70°-80°	80°-90°
266 lm	779 lm	1145 lm	1216 lm	1110 lm	891 lm	578 lm	316 lm	160 lm
90°-100°	100°-110°	110°-120°	120°-130°	130°-140°	140°-150°	150°-160°	160°-170°	170°-180°
84,9 lm	74,9 lm	56,1 lm	45,1 lm	33,6 lm	21,3 lm	12,0 lm	5,87 lm	1,69 lm

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](#)

Operator:



## Outdoor Light Planning

### Lumen per Zone

Zone (γ)	Lumen	% Total
0-10°	266 lm	3,9%
10-20°	779 lm	11,5%
20-30°	1145 lm	16,8%
30-40°	1216 lm	17,9%
40-50°	1110 lm	16,3%
50-60°	891 lm	13,1%
60-70°	578 lm	8,5%
70-80°	316 lm	4,6%
80-90°	160 lm	2,4%
90-100°	85 lm	1,2%
100-110°	75 lm	1,1%
110-120°	56 lm	0,8%
120-130°	45 lm	0,7%
130-140°	34 lm	0,5%
140-150°	21 lm	0,3%
150-160°	12 lm	0,2%
160-170°	6 lm	0,1%
170-180°	2 lm	0,0%
<b>Total</b>	<b>6797 lm</b>	<b>100,0%</b>

### Intensity peaks

Max intensity	2816 cd
Intensity, 90°	98 cd
Intensity, 0°	2816 cd

### Zonal Lumen summary


Zone (γ)	Lumen	% Total
0-30°	2191 lm	32,2%
0-40°	3407 lm	50,1%
0-60°	5408 lm	79,6%
60-90°	1053 lm	15,5%
70-100°	561 lm	8,2%
90-120°	216 lm	3,2%
0-90°	6461 lm	95,1%
90-180°	335 lm	4,9%
0-180°	6797 lm	100,0%

### BUG rating

	Lumen	% Total
<b>Forward light</b>		
Low(0-30°)	1093 lm	16,1%
Medium(30-60°)	1608 lm	23,7%
High(60-80°)	448 lm	6,6%
Very high(80-90°)	80 lm	1,2%
<b>Back light</b>		
Low(0-30°)	1093 lm	16,1%
Medium(30-60°)	1608 lm	23,7%
High(60-80°)	448 lm	6,6%
Very high(80-90°)	80 lm	1,2%
<b>Uplight</b>		
Low(90-100°)	86 lm	1,3%
High(100-180°)	250 lm	3,7%

## IESNA TM-15-07 Luminaire Classification System For Outdoor Luminaires

**BUG rating B3 U3 G1**

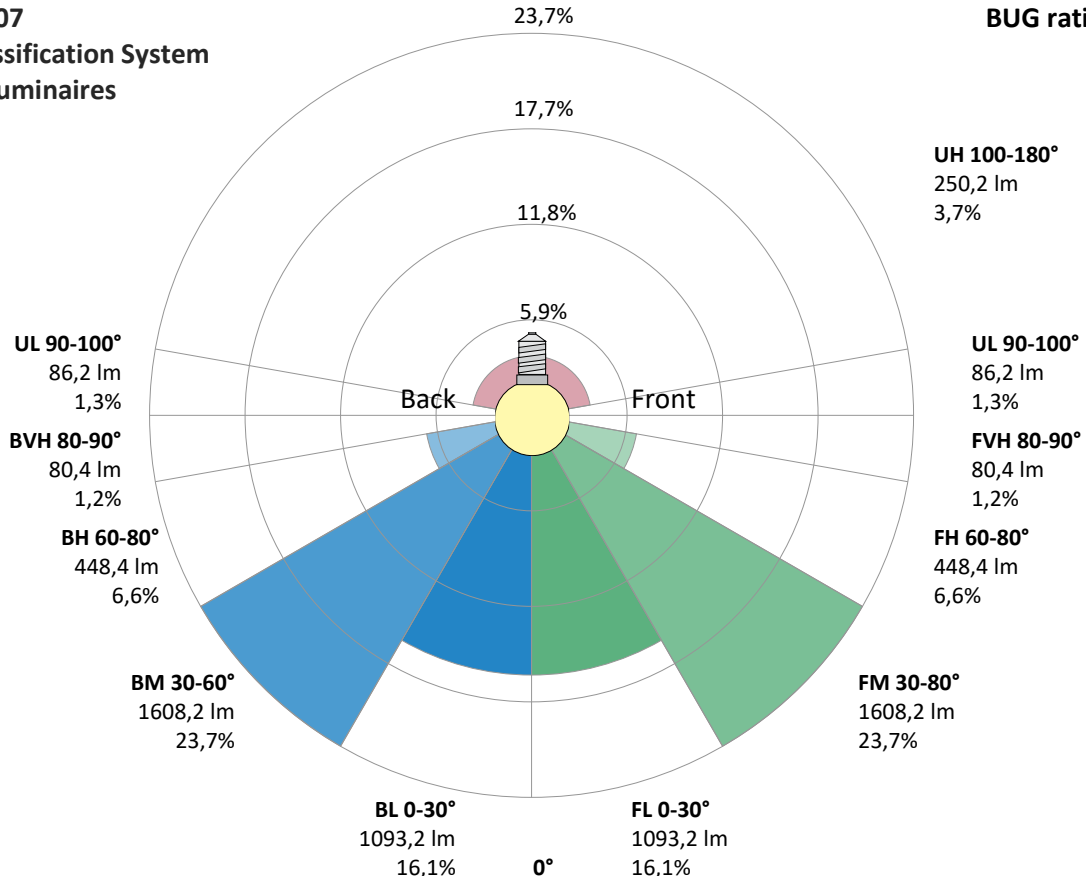

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](#)

Operator:




## Power Details


### Input Power

Power feed to light source	50,4 W
Frequency of input power	50 Hz
RMS Input voltage feed, $V_{RMS}$	230 V
RMS Input current feed, $I_{RMS}$	0,227 A
Volt-Ampere or apparent power = $V_{RMS} * I_{RMS}$	52,14 VA
Displacement factor of AC power feed	0,97
Power factor of AC current feed	0,97
Total harmonic distortion of the current	6,56%
Total harmonic distortion of the voltage	0,06%

### Input Power Curve

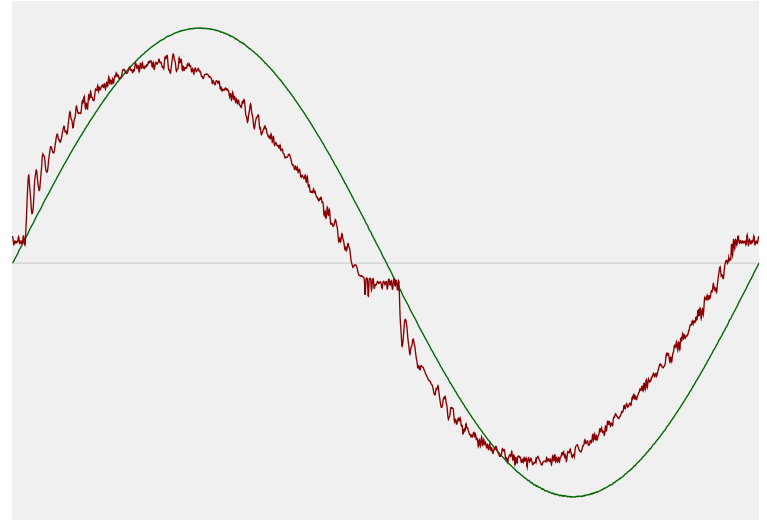

### Efficiency

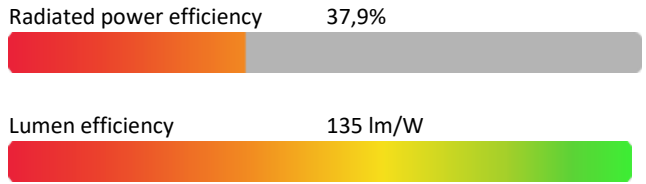

## Stabilization Details

### Warmup Conditions

Stable period	15 min
Stable change max	2,0%
Minimum time	15 min

### Color Temperature Change

CCT start	3002 K
CCT shift	-2 K
CCT end	3000 K


### Warmup Result

Total warmup time	Lamp stabilized in 15 min 1 sec
Warmup variation	-0,3%

### Output Change

Output start	6813 lm
Output change	-16 lm
Output end	6797 lm

### Stabilization Curve

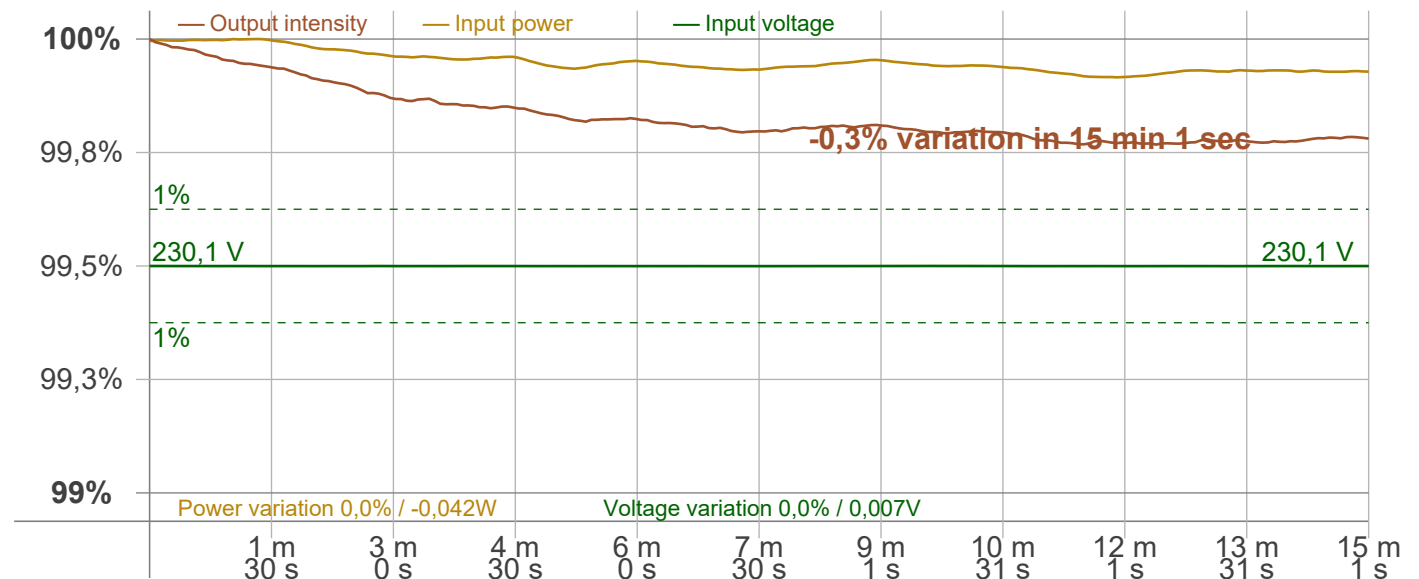

# Light Measurement Report

Print date: 29-10-2025

Measurement date and time: 29-10-2025 11:33:27 – Measurement no. VFR-251029-3812-MS

Measurement tracking No. and Link: [VT251029-003886](https://www.viso-systems.com/VT251029-003886)

Operator:



## Flicker /TLA details

Flicker Meter Type Viso Systems LabFlicker  
 Frequency of input power 50 Hz  
 Flicker/TLA sample rate 20000 samples/s

**Measurement time**  
 PstLM 180 sec  
 All other indices 1,2 sec

### Flicker indices according to Illuminating Engineering Society (IES)

Flicker frequency 100,5 Hz  
 Percent Flicker 0,19 %  
 Flicker index 0

### Flicker indices according to California Energy Commission (CEC) 2016b

JA8/10 40 Hz 0,03 %  
 JA8/10 90 Hz 0,03 %  
 JA8/10 200 Hz 0,07 %  
 JA8/10 400 Hz 0,09 %  
 JA8/10 1000 Hz 0,15 %


### TLA indices (re IEC TR 61547-1, IEC 61000-3-3 and IEC 61000-4-15)

PstLM value (F < 80 Hz) 0,02  
 SVM value (80 < F < 2000 Hz) 0

### Flicker indices according to Lighting Research Center (2015)

Perception metric, Assist Mp 0,01

### Flicker frame (frame of one flicker period in time domain)

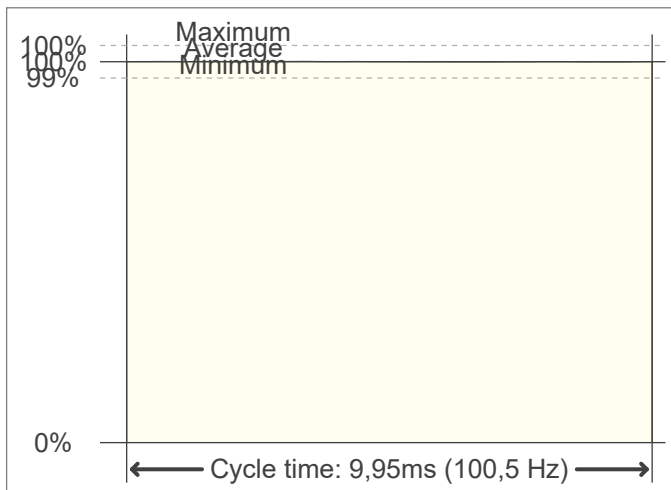

### Flicker FFT (flicker curve in frequency domain)



### IEEE 1789 Frequency/modulation plot

